Umano Medical

A Main Nurse Control
- Lock out
- Bed movements
- Scale & bed exit
- Battery indicator

B Bed Exit Sideview Lights
(on foot bumpers)
- Green = Armed
- Flashing amber = In alarm
- Not illuminated = Alarm is OFF

C Bed extender (optional)
- Reach & pull on Green handle
- Pull to extend
- Push to retract
- Set to desired length and lock
- Install cushion

D Siderail Controls
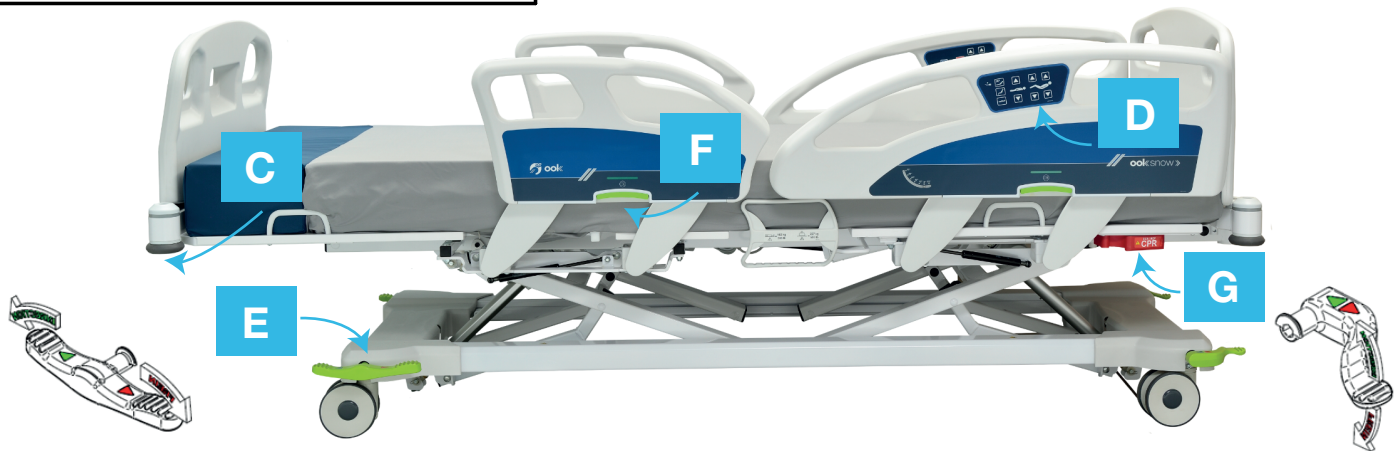- Outside of siderail = nurse controls
- Inside of siderail = patient controls

Siderail controls can be locked at foot end

BED OVERVIEW

Reminders

- Ensure bed is plugged to enable scale, bed exit & advanced features

- Apply the brakes

E Brake Pedals
- Push Red = Brake ON
- Push Green = Steer ON
- Horizontal = Neutral position (Bed is fully mobile)

F Siderail Release
- Lift green handle UP to unlock
- Lower siderail down

Green window indicates safe status
Red window indicates unlocked siderail

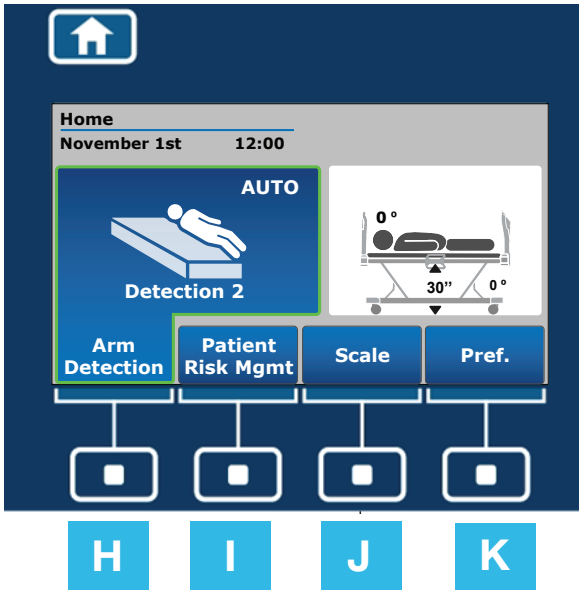## G CPR Release Handle
- Pull red handle
- Completely lower backrest section

Seat section will automatically retract flat. Press any button to cancel

*Please refer to the user manual for **detailed instructions**, safety measures and warnings.*

SCALE & BED EXIT

HOME Button on the footboard returns the display to HOME SCREEN / MAIN MENU

NAVIGATION Buttons on footboard will activate commands on MENU

Home
November 1st   12:00

AUTO

Detection 2

0 °
30"   0 °

| Arm Detection | Patient Risk Mgmt | Scale | Pref. |

H I J K

## H — To arm/disarm BED EXIT system (Regular/Manual setting)

① To arm BED EXIT:
Patient must be in bed to arm bed exit system. From HOME SCREEN,
   Press 'ARM' **H**
   Press 'YES' ('to arm bed exit')
Verify that foot end bumper indicators (optional) are illuminated green. When foot bumpers are illuminated green, bed exit system is 'ARMED'.

② To disarm BED EXIT (if alarm is triggered) :
Press 'DISARM' (on the HOME SCREEN). This will turn 'OFF' the alarm. Patient must be placed back in bed and alarm must be manually REARMED.

I — To change BED EXIT detection level

Please note bed alarm must be 'OFF' to make changes.

To change or set DETECTION LEVEL
From the HOME SCREEN,   Press **Patient Risk Mgmt**
                    Press **Select**
Press **→** to scroll through detection level options and Press 'Select detection' to select desired level.

Patient Risk Management
November 1st   12:00
Info | Set Detection | Alarm Settings
Select   Close

Bed Exit Detection settings
November 1st   12:00
Detection | Detection 2 | Detection 3
Auto Arm → Select detection Close

J — To 'ZERO' out the SCALE

From the HOME SCREEN
Press 'SCALE' button
Press **→** (Press once to scroll to 'Zero')
Press **Select** to 'ZERO'

Press 'START' to confirm
Important: Patient should not be on bed during procedure.

Scale
November 1st   12:00
Weigh | Zero | Detailed Weight
← → Select Close

Zero
November 1st 12:00
Patient shall not be on bed. Install equipment.
Undo Zero   Start Cancel

J — SCALE - To weigh patient

From the HOME SCREEN, Press 'SCALE' button
Press 'SELECT'
Press 'Weigh' to display weight **Weigh**

Weight log screen informs of patient logged weight

160.5 Lb
72.8 Kg
Weigh Close Clone

Weight Log
November 1st   12:00
Weight/Lb
190.3 190.5 190.9 190.7 190.8 190.8 Date
Logged weight: Nov 1st 2014 12:00
← → Erase Close

K — Preference menu

Lights configuration, Lockouts, ID, Auto-contour, Minimum height adjustment, Date/time, Languages, Maintenance

H — To arm/disarm BED EXIT system (AUTO Arm) **Auto Arm**

When Auto Arm is activated and patient is detected in bed, the bed exit is armed automatically.

To disarm BED EXIT (if alarm is triggered) :
   Press 'DISARM' (which will appear on the HOME SCREEN). This will turn 'OFF' the alarm.
If patient is out of bed :
   The system will return to stand-by mode.
If patient is still in bed :
   The system will apply a 1-minute care PAUSE to the auto-arm to allow the caregiver to attend to the patient. If after 1 minute patient is still in bed, the system will automatically initiate arming procedure.

I — To turn on/off AUTO Arm

From Home Screen, Press **Patient Risk Mgmt**
Press 'Select' to enter Select detection menu
Press 'Auto Arm' to activate or deactivate it

I — To change ALARM settings
(Volume and tone) 🔊 🎵

Alarm **must be OFF** to change settings.
From the HOME SCREEN
   Press 'Patient Risk Mgmt'
   Press **→**
   Press 'Select' to enter Alarm Settings menu. Make desired changes and press 'OK' to save changes.

For immediate assistance, please contact your local account executive.

*Please refer to the user manual for **detailed instructions**, safety measures and warnings.*